

526,279

(12) INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(19) World Intellectual Property
Organization
International Bureau



01 MAY 2005

(43) International Publication Date
1 April 2004 (01.04.2004)


PCT

(10) International Publication Number
WO 2004/026191 A1

- (51) International Patent Classification⁷: **A61F 2/46**
- (21) International Application Number:
PCT/AU2003/001229
- (22) International Filing Date:
19 September 2003 (19.09.2003)
- (25) Filing Language: English
- (26) Publication Language: English
- (30) Priority Data:
2002951548 19 September 2002 (19.09.2002) AU
- (71) Applicant (for all designated States except US):
FLINDERS TECHNOLOGIES PTY. LTD. [AU/AU];
Mark Oliphant Building, Laffer Drive, Science Park
Adelaide, Bedford Park, South Australia 5042 (AU).
- (72) Inventor; and
(75) Inventor/Applicant (for US only): **KRISHNAN, Je-
ganath** [AU/AU]; 19 Thornber Street, Unley Park, South
Australia 5061 (AU).
- (74) Agent: **DAVIES COLLISON CAVE**; PRYOR, Geoffrey,
Charles, **LESLIE**, Keith, **WEBBER**, David, Brian, 1 Little
Collins Street, Melbourne, Victoria 3000 (AU).
- (81) Designated States (national): AE, AG, AL, AM, AT, AU,
AZ, BA, BB, BG, BR, BY, BZ, CA, CH, CN, CO, CR, CU,
CZ, DE, DK, DM, DZ, EC, EE, EG, ES, FI, GB, GD, GE,
GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR,
KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD, MG, MK,
MN, MW, MX, MZ, NI, NO, NZ, OM, PG, PH, PL, PT,
RO, RU, SC, SD, SE, SG, SK, SL, SY, TJ, TM, TN, TR,
TT, TZ, UA, UG, US, UZ, VC, VN, YU, ZA, ZM, ZW.
- (84) Designated States (regional): ARIPO patent (GH, GM,
KE, LS, MW, MZ, SD, SL, SZ, TZ, UG, ZM, ZW),
Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM),

[Continued on next page]

(54) Title: IMPLANT CLAMP AND METHOD

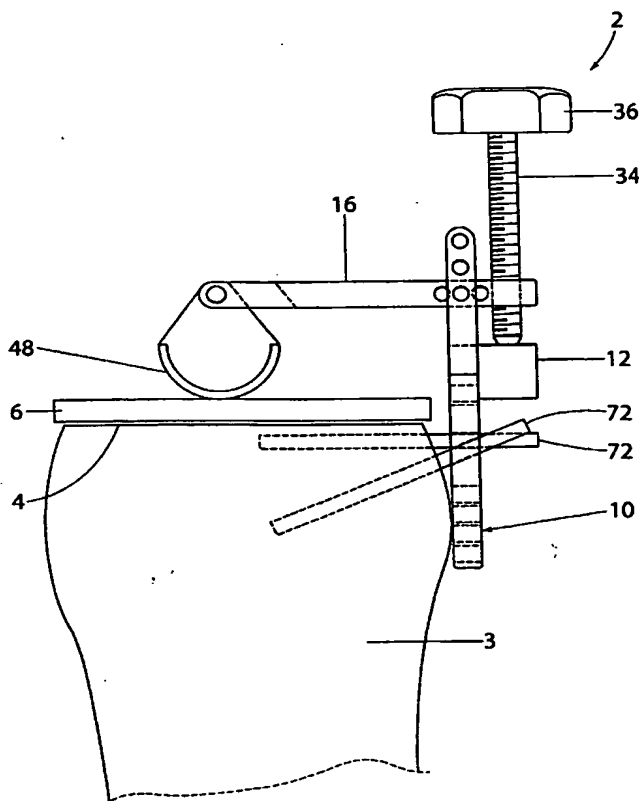

(57) **Abstract:** An implant clamp for clamping an im-
plant having a base to a bone. The clamp includes a
support (10), a means to couple the support to the bone
(72), an arm (16) pivotally connected to the support and
an actuating member (36) operable to cause rotation of
the arm relative to the support member. The arm exerts
a force on the implant that is substantially perpendicular
to the base.

WO 2004/026191 A1